


| | | | |
|----------|----------------|--------|-----------|
| Name | Sample_Initial | | |
| Birthday | 1993.1.1 | Gender | Female |
| X-Ray | 2007.5.3 | Norm | Caucasian |
| Age | 14yr 4mo | Case | 12345 |

Steiner Analysis

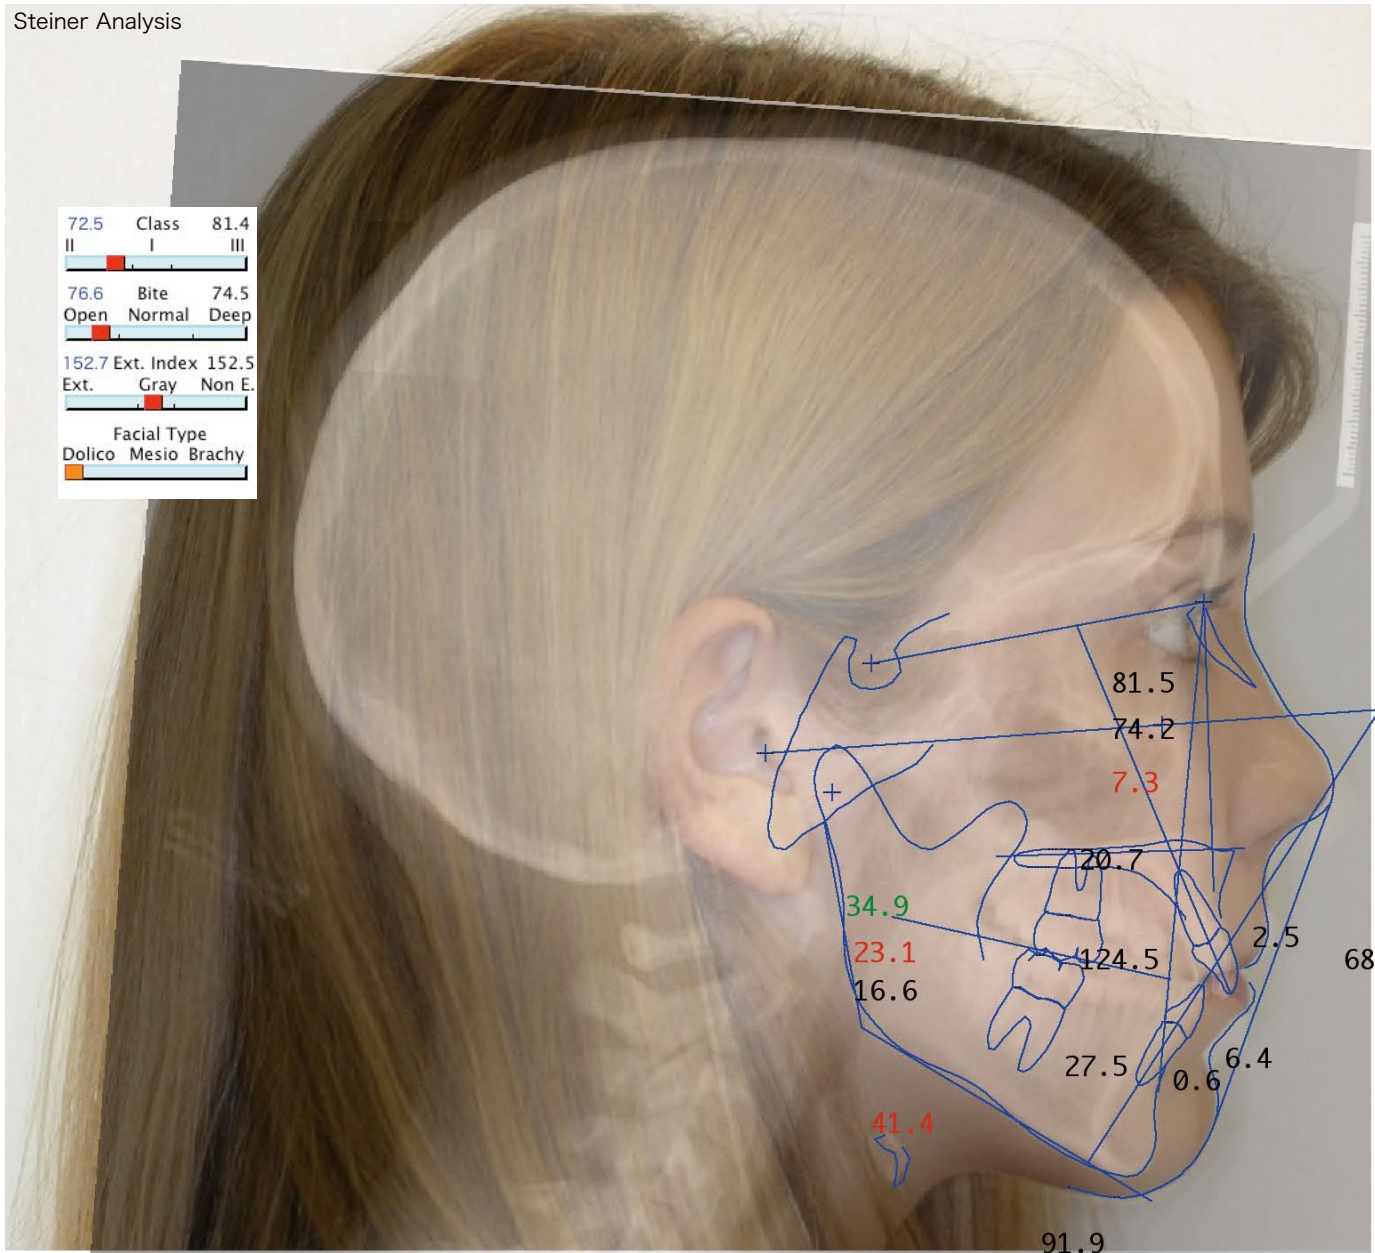

| Measurements | Patient | Mean | S.D. | C.D. |
|---------------------|---------|------|------|------|
| SNA | 81.5 ° | 82.0 | 3.0 | |
| SNB | 74.2 ° | 80.0 | 3.0 | * |
| ANB | 7.3 ° | 2.0 | 2.0 | ** |
| Mx1-NA | 2.5 mm | 4.0 | 3.0 | |
| Mx1-NA Angle | 20.7 ° | 22.0 | 6.0 | |
| Md1-NB | 6.4 mm | 4.0 | 3.0 | |
| Md1-NB Angle | 27.5 ° | 25.0 | 6.0 | |
| PO - NB | 0.6 mm | 1.0 | 1.8 | |
| Occlusal Plane - SN | 23.1 ° | 14.0 | 3.5 | ** |

| Measurements | Patient | Mean | S.D. | C.D. |
|-------------------------|---------|-------|------|------|
| GO-GN-SN | 41.4 ° | 32.0 | 4.5 | ** |
| Interincisor Angle | 124.5 ° | 130.0 | 6.0 | |
| Wits Appraisal | 2.1 mm | 1.1 | 1.9 | |
| Adjusting ANB (FREEMAN) | 7.8 ° | 2.0 | 2.0 | ** |
| FMA | 34.9 ° | 25.0 | 6.0 | * |
| FMIA | 53.2 ° | 65.0 | 6.0 | * |
| IMPA | 91.9 ° | 90.0 | 6.0 | |
| Occlusal Plane - FH | 16.6 ° | | | |
| Z Angle | 68.9 ° | | | |

